

Supplementary Materials: A Skin-Conformal, Stretchable, and Breathable Fiducial Marker Patch for Surgical Navigation Systems

Sangkyu Lee, Duhwan Seong, Jiyong Yoon, Sungjun Lee, Hyoung Won Baac, Deukhee Lee and Donghee Son

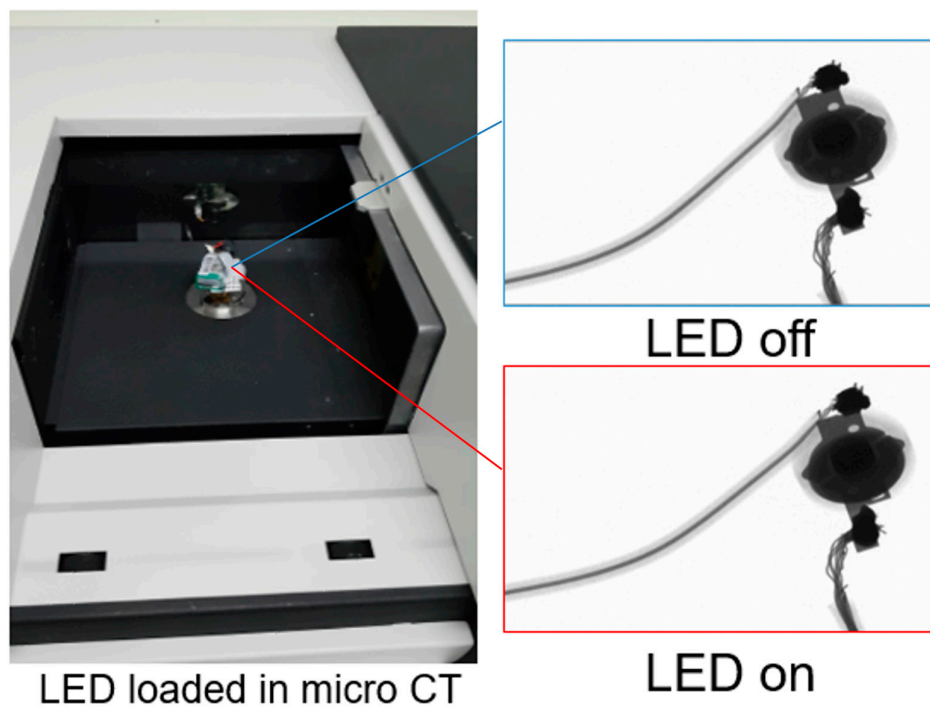


Figure S1. X-ray stability and recognition of the micro-IR LED with a micro-CT machine.